

Chromatogram Report



Analysis Info

Analysis Name D:\Data\test\MK667_1-F,1_01_57792.d
 MS Method peptide-with_ms.m
 Sample Name MK667
 Comment

Acquisition Date Dec/20/2017 2:25:25 PM
 Operator Microtof
 Instrument UPLC No.1

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.0 Bar
Focus	Active			Set Dry Heater	180 °C
Scan Begin	100 m/z	Set Capillary	4500 V	Set Dry Gas	2.0 l/min
Scan End	3000 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Waste

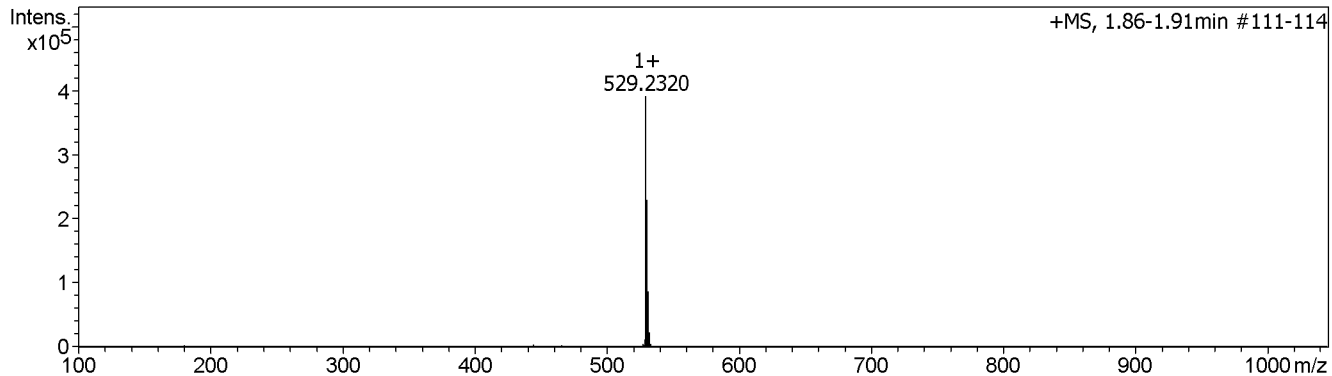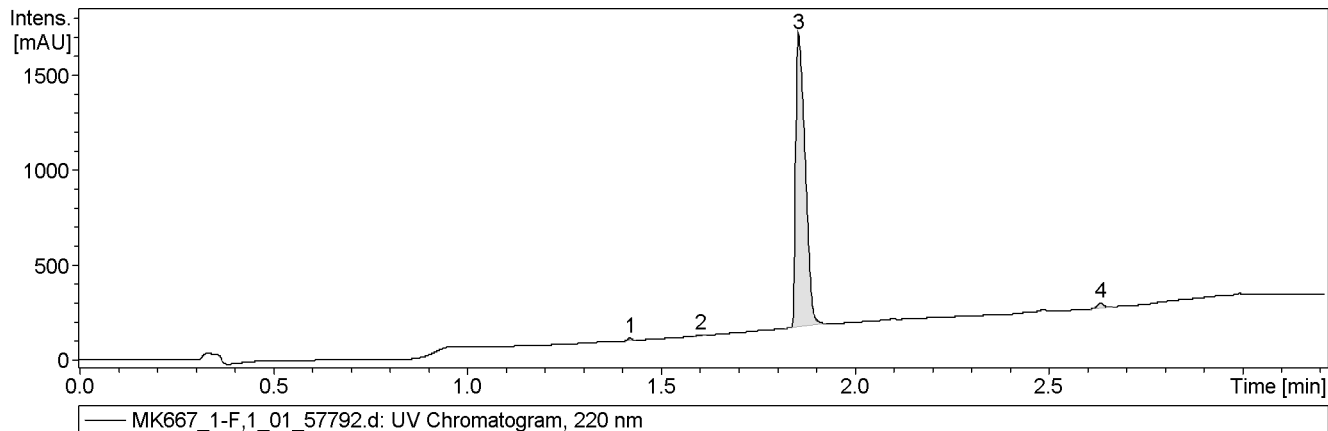

#	RT [min]	Area	Int. Type	I	S/N	Chromatogram	Max. m/z	Area Frac. %
1	1.42	9.2624	Manual	114	114.3	UV Chromatogram, 220 nm	0.0000	0.36
2	1.60	4.5231	Manual	132	52.5	UV Chromatogram, 220 nm	0.0000	0.18
3	1.86	2538.0098	Chromatogram	1717	1926.7	UV Chromatogram, 220 nm	0.0000	98.21
4	2.63	32.3598	Manual	300	246.5	UV Chromatogram, 220 nm	0.0000	1.25
n.a.	1.88	n.a.	Average spectrum	n.a.	n.a.	n.a.	529.2320	n.a.