

CDSolutions

APPLICATIONS INFORMATION USING ADVANCED SAMPLE HANDLING TECHNOLOGY

Evaluation of Source Rock using EGA and Pyrolysis GC/MS

To understand the organic matter of sedimentary rock as an evaluation of potential fuel output, geochemists use techniques which involve heating the rock to determine the amount of free hydrocarbons, and the amount of hydrocarbons and fixed gases are produced during thermal cracking. With the Pyroprobe, the quantity of these products can be determined, as well as their chemical nature. First the rock is heated to 300°C, and resulting hydrocarbons are transferred to a GC-MS for separation and identification (Figure 1). After the first GC run is completed, the procedure is repeated a second time, but heating to 600°C to release cracking products (Figure 2).

Migratory Hydrocarbons and Thermal Cracking composite peaks can be determined by replacing the GC column with a one-meter length of 0.1 mm fused silica, and keeping the GC at 300°C. This is shown in Figure 3. As the rock is heated, hydrocarbons from the rock are transferred rapidly to the detector as they are made. The interfacing, inlet pressure and split ratio are used just as they would be for GC-MS analysis, but rather than producing a chromatogram of individual compounds, the results are composite peaks of the materials made during the heating process.

Figure 3 also shows a value for Tmax (508°C). This is the temperature at which the most hydrocarbons are released during thermal cracking. Fixed gases created during thermal cracking can also be determined by interfacing CDS Model 5500 Fixed Gas Analyzer to the vent of the Pyroprobe (not shown).

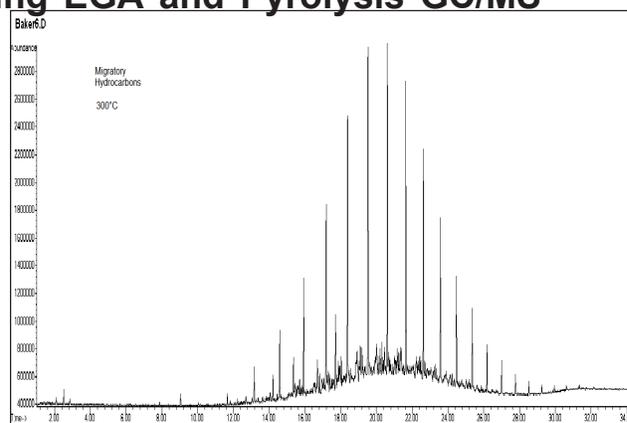


Figure 1: Migratory Hydrocarbons of Source Rock.

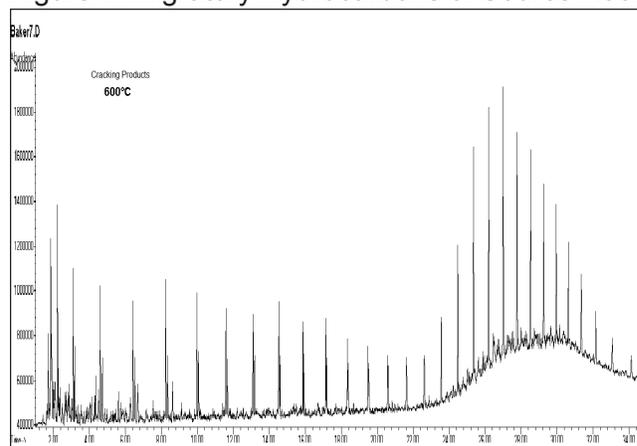


Figure 2: Cracked Hydrocarbons of Source Rock.

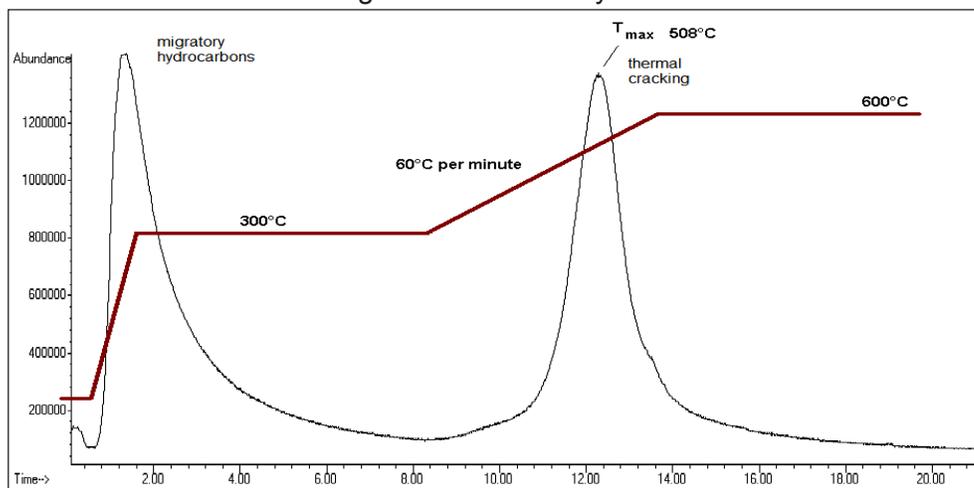


Figure 3: Composite Peaks of Source Rock.

Equipment

This sample was analyzed using a CDS Model 5200 Pyroprobe interfaced to a gas chromatograph/mass spectrometer.

Model 5200 Conditions (GC/MS Analysis)

Interface:

Initial: 50°C
Final: 300°C 4 minutes

Trap:

Initial: 50°C
Final: 300°C

Probe Coil: 300°C or 600°C for 1 min

Transfer Line: 325°C
Valve Oven: 300°C

GC Conditions (GC/MS Analysis)

Carrier: Helium
Injector: 300°C
Split: 50:1
Column: 5% phenyl (30m X 0.25mm)
Detector: MS
Range: 35 - 550

GC Program:

Initial: 40°C for 2 minutes
Ramp: 10°C/min.
Final: 300°C

Model 5200 Conditions (Composite Peaks)

Interface:

Rest: 60°C
Initial: 60°C
Ramp: 60°C per minute
Final: 300°C

Pyroprobe:

Initial: 300°C (6 minutes)
Ramp: 60°C per minute
Final: 700°C

Transfer Line: 300°C

Valve Oven: 300°C

GC Handshaking must be turned off, GC manually started when Pyroprobe method is started.

GC Conditions (Composite Peaks)

Carrier: Helium
Injector: 300°C
Split: 50:1
Column: fused silica 1m, .1mm ID
Detector: MS
Range: 35 - 550

GC Program:

Initial Hold: 300°C for 20 minutes

CDS Analytical, Inc. has been a leader in the design and manufacture of laboratory instruments for sample preparation and analysis since 1969. We are dedicated to providing the best possible instruments for both research and routine analysis. Well known in the field of pyrolysis, CDS manufactures the Pyroprobe 5000, 5150, 5200 and 5250 autosampler for the introduction and analysis of solid materials by GC, MS and FT-IR. CDS offers a complete line of dynamic headspace instruments for the analysis of volatile organic compounds in environmental, pharmaceutical and food applications as well as purge & trap instruments for drinking and waste water. CDS also manufactures the Dynatherm line of thermal desorption instruments including the 9300 series for air monitoring and the 7500 autosampler. Our customers, their requirements and applications are important to us. To help meet your needs, we offer a wide range of analytical information and the services of our applications laboratory. If you would like additional information, please contact us at the address below, call us at 1 800 541 6593, or log onto www.cdsanalytical.com.